

# Proposal of a P300-based BCI Speller using a Predictive Text System

Ricardo Ron-Angevin and Leandro da Silva-Sauer

*Departamento de Tecnología Electrónica, E.T.S.I. Telecomunicación  
University of Málaga, Campus de Teatinos s/n, 29071 Málaga, Spain*

**Keywords:** Brain-computer Interface (BCI), P300, Speller, T9 Interface.

**Abstract:** This paper presents a P300-based BCI speller system that uses a virtual 4 x 3 keyboard based on the T9 interface developed on mobile phones in order to increase the writing speed. To validate the effectiveness of the proposed BCI, we compared it with two adaptations of the classical Farwell and Donchin speller, which is based on a 6 x 6 symbol matrix. Three healthy subjects took part in the experiment. The preliminary results confirm the effectiveness of T9-based speller, since the time needed to spell words and complete sentences was considerably reduced.

## 1 INTRODUCTION

Brain-computer interface (BCI) systems (Wolpaw et al., 2002; Birbaumer, 2006) are devices that transform a user's brain activity into commands that are interpreted by a machine. Such systems offer a non-muscular channel for users to interact with their environment. This is particularly useful for people suffering from neurodegenerative disorders, such as amyotrophic lateral sclerosis, as they can eventually present severe motor disabilities, to the point of losing control of the muscles that are responsible of voluntary body movements, including eye movement and breathing itself. In those cases, BCIs turn out to be the only way for patients to gain some degree of communication and autonomy in their daily lives.

The most widely used BCI systems are those based on electroencephalographic (EEG) signal recording, due to its non-invasiveness, but also to its good temporal resolution and ease of use. Three types of EEG-based BCI systems have been used for communication purposes, namely those based on: (a) slow cortical potentials (SCPs), (b) P300 event-related potentials (ERP), and (c) sensorimotor rhythms (SMR) (Mak and Wolpaw, 2009). BCIs based on SCP and SMR demand that users are extensively trained before they show sufficient control of their brain activity. In contrast, BCIs based on P300 rely on a common, expected human response to infrequent target stimuli—usually visual—and thus require minimal training. The P300 signal, recorded over the central and parietal regions, is a positive deflection of

brain wave at a latency of about 300 ms after stimulus presentation.

The main applications of P300-based BCI systems are aimed at communication purposes. They are based on the P300 speller first developed by Farwell and Donchin (1988), which is still referenced and intensely studied (Bianchi et al., 2010; Kleih et al., 2010; Krusienski et al., 2008; Sellers et al., 2006). In this BCI, a 6 x 6 matrix of letters, arranged in rows and columns, is shown to the subject. The user focuses his/her attention on the matrix element he/she wishes to select as each row and column is flashed (i.e., intensified) randomly, one after the other. After a number of flashes, the symbol that the user was supposedly attending at is presented on screen.

The effectiveness of the P300-based BCI speller system is guaranteed by a number of studies carried out not only on healthy subjects (Donchin et al., 2000; Wang et al., 2005) but also on subjects affected by some motor disability (Sellers and Donchin, 2006). Overall, these studies conclude that the P300 speller processor is an effective communication tool for people who have lost or are losing their ability to write or speak. However, it is still needed to improve the usability of these BCI speller systems. Some factors, such as the mental fatigue induced by a long use (Kececi et al., 2006; Murata and Uetake, 2001), the sustained attention at a symbol on screen (Mangun and Buck, 1998), the user motivation (Kececi et al., 2006; Kleih et al., 2010) or his/her frustration due to a mistake (Kleih et al., 2010) can influence the amplitude and latency of the P300 component (See Polich and

Kok, 1995, for a review). In this regard, the influence on performance of the temporal and spatial aspects of the user interfaces of these systems is increasingly drawing the attention of researchers (Lu et al., 2013; McFarland et al., 2011; Shih et al., 2013)

This paper presents a study aimed at contributing to this line of research. We propose a P300-based BCI speller system that uses the T9 interface developed for mobile phones (Grover et al., 1998). Specifically, the virtual keyboard of this interface consisted of a 4 x 3 matrix that was based on that of the T9 interface. Compared to the 6 x 6 matrix used by conventional P300-based spellers (Donchin et al., 2000), using a smaller matrix was expected not only to lead to a higher accuracy, but also to reduce the time required to select a character, since the number of rows and columns that had to be flashed to detect it was reduced. On the other hand, we provided this speller with a text predictive system because selecting some characters in a 4 x 3 matrix would demand more than one choice from the user. Such a system would render those extra choices hardly unnecessary and thus increase the user's writing speed (as discussed by Dulong and Crossan (2000)). To validate the effectiveness of the proposed BCI, we compared it with two adaptations of the classical Farwell and Donchin speller in terms of the time needed to write a target sentence.

## 2 METHOD

### 2.1 Participants, Procedure and Data Acquisition

Three healthy subjects (one man, aged 36, and two women, aged 22 and 25) took part in the experiment. None of them had previous experience with BCI systems. The experiment was divided into three sessions. The objective of each session was to evaluate one of the proposed interfaces, namely the two adaptations of the classical speller (i.e., the *Spellermod* and the *SpellermodPred*) and a speller based on the T9 interface (i.e., the *SpellerT9*). A description of these three interfaces will be done in the following sections.

Each participant carried out the three sessions in different days. To avoid effects due to learning, the order in which participants completed the three sessions was randomized.

Each session was divided into two phases: a first one for calibration purposes and a second one to evaluate the interface. Participants were instructed to silently count how many times the selected symbol was intensified (i.e., flashed). In the calibration phase,

they were asked to copy five sequences of three to four characters. In the evaluation phase, they were asked to write the sentence "Experiencia BCI en la Universidad de Málaga" (i.e., BCI experience at the University of Málaga).

As we wanted to compare the three interfaces in terms of the writing speed their users could achieve, the values of all the temporary parameters related to the selection of a symbol (i.e., a letter) were equal across them. These values were based on those used by Donchin et al. (2000). Specifically, each row and column was randomly flashed 10 times. Therefore, each character was randomly intensified 20 times. The duration of each flash was 125 ms and the inter-stimulus interval (ISI) between flashes was also 125 ms. There was a pause of 2 s after each sequence of flashes (i.e., after a character had been selected) and also in the beginning of each trial. It is important to notice that the duration of a sequence of flashes depended on the size matrix, so that bigger matrices entailed longer sequences.

Eight-channel EEG data were recorded at the electrodes Fz, Cz, Pz, Oz, P3, P4, PO7 and PO8—according to the 10/20 international system—, with FPz as reference and the left mastoid as ground. Data were acquired by a biosignal amplifier (g.BSamp, Guger Technologies) with a sampling rate of 256 Hz and a 12-bit resolution data acquisition NI-USB-6210 (National Instruments) card.

### 2.2 System Description

The three P300-based spellers were implemented through the BCI2000 platform (Schalk et al., 2004). The first speller, called *Spellermod*, was an adaptation of the classical Farwell and Donchin speller. Unlike this, which consisted of a 6 x 6 symbol matrix, the *Spellermod* presented a 7 x 6 virtual keyboard, in which additional symbols were included. We will refer to the *Spellermod* as the reference speller. The second speller, called *SpellermodPred*, was identical to the previous one, save for the fact that the *SpellermodPred* included a text predictive system in order to reduce the time needed to write. Finally, the third speller, called *SpellerT9*, consisted of a small 4 x 3 symbol matrix and included the same text predictive system used in the *SpellermodPred*. Next, we give a better description of these interfaces.

#### 2.2.1 Spellermod

The *Spellermod* used a 7 x 6 matrix (See Figure 1). The last row contained only two special characters, *BORRAR* and *ESPACIO*, for deleting a character and introducing a blank space, respectively. Therefore,

in case of a spelling error, the user was able to erase the last letter by selecting the special character BORRAR. Besides, the digit zero was also included in the sixth row.

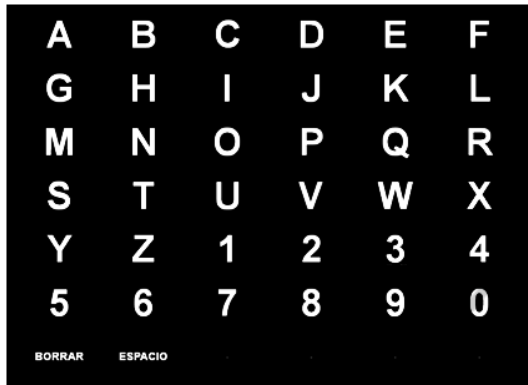


Figure 1: Interface of the Spellermod.

The characters that the user had selected were displayed inside a text box situated at the bottom of the screen. According to the temporary parameters described in section 2.1, the time needed to select a symbol through this interface was 34.5 s—the initial 2 s of pause plus the duration of flashing seven rows and six columns 10 times each during 125 ms with an ISI of 125 ms—.

### 2.2.2 SpellermodPred

Although the main objective of this study was to compare the SpellerT9 with the reference speller (i.e., the Spellermod), we considered very interesting to assess the performance of a classical speller when it included a text predictive system. So, we developed the SpellermodPred speller (See Figure 2). Its interface was like the Spellermod's 7 x 6 matrix, only now it included the special character *VALIDAR*. Since the matrix dimensions were the same as in the Spellermod, the time needed to select a symbol using the SpellermodPred was also 34.5 s.

The characters (i.e., letters) that the user selected were displayed in a text box below the symbol matrix. These characters were fed into the text predictor, which in turn displayed the most frequently used Spanish word starting with those letters in an additional text box, just above the former. For example, if the subject had selected the letter G and then the letter O, the predictor would suggest the word *gobierno* (i.e., the Spanish word for government).

In case the suggested word were the one the user wanted to write, he/she could confirm it by selecting the special character *VALIDAR*. As a consequence, the rest of the word was added to the letters he/she had already spelled, allowing the user to write a new

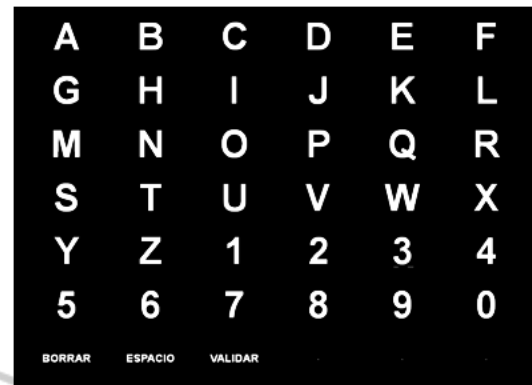


Figure 2: Interface of the SpellermodPred.

word. Importantly, validating a word also added a blank space at the end of it.

The list of the most frequently used Spanish words was obtained from the Royal Spanish Academy. In case of wanting to write in a different language, it would only be necessary to change the dictionary used by the text predictor.

### 2.2.3 SpellerT9

The SpellerT9 used the T9 predictive text system developed for mobile phones. Its interface (See Figure 3) consisted of a 4 x 3 matrix of elements or *keys*, in which only eight keys—the ones corresponding to the numbers 2 to 9—were used for spelling. Each of those keys corresponded to three to four letters. Importantly, as the matrix size was 4 x 3, the time needed to select a symbol in the SpellerT9 was just 19.5 s—the initial 2 s of pause plus the duration of flashing four rows and three columns 10 times each during 125 ms with an ISI of 125 ms—, less than that of the other spellers.

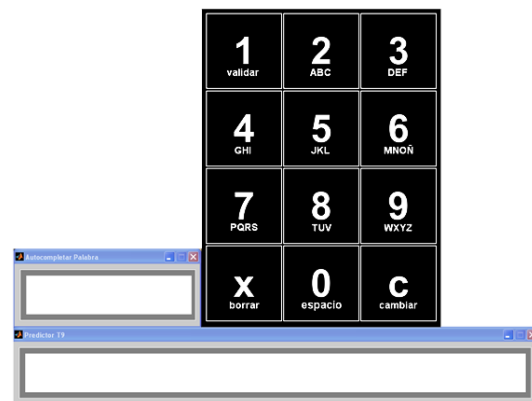


Figure 3: Interface of the SpellerT9.

As in the T9 interface of mobile phones, the user of the SpellerT9 had to select a sequence of the men-

tioned eight keys in order to write a word. As the user selected a sequence of those keys, the most favorable sequence of letters corresponding to those keys was displayed in the text box at the bottom of the interface. To increase writing speed, the SpellerT9 used a text predictive system, exactly like the one used in the SpellermodPred. This system identified the four more frequently used Spanish words starting with the suggested sequence of letters. The most frequent of them was displayed in the text box beside the keyboard and the other three were kept in memory. For example, after selecting the sequence of keys 2272, the four predicted words would be *casa*, *cara*, *capa*, and *basa*, being *casa*—the most frequently used—the one displayed beside the keyboard. In case that were the word that the user wanted to write, he/she could confirm it by selecting the key 1 (i.e., *validar*). This, as in the SpellermodPred, added a blank space at the end of the word. Otherwise, the user could select the key c (i.e., *cambiar*) to switch to a new interface that displayed the four predicted words (See Figure 4). The user could then select one of them or alternatively go back to the virtual keyboard by selecting the left arrow key (i.e., *volver*).

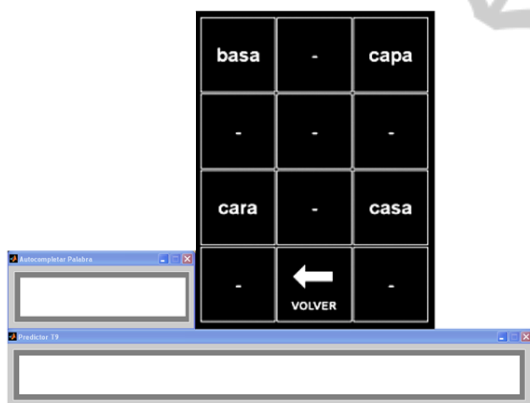


Figure 4: 4 x 3 matrix of the SpellerT9 showing the four most frequently used Spanish words associated with the sequence of keys 2272.

Like in the other two spellers, users could delete characters—by selecting the key x (i.e., *borrar*)—or include blank spaces—by selecting the key 0 (i.e., *espacio*)—. The SpellerT9 made it also possible for users to write digits. To do so, he/she had to select the key c prior to selecting any letter of a new word. In this way, the user could select the keys 0 to 9 to write the corresponding digits. Once the desired digits had been written, the user had to select the key c again to continue writing words.

### 3 RESULTS AND DISCUSSION

The spelling times needed by each of the three participants to write the target sentence (i.e., “Experiencia BCI en la Universidad de Málaga”) through each of the three compared spellers are shown in Table 1. We did not discount the times associated with errors. The table also displays the minimum required times that a perfect user (i.e., a user that selected each character at the first attempt) would need to write the target sentence in each case.

As we can see, the three participants wrote nearly all words faster with the SpellerT9 than with any of the other two spellers. Even participant 2, who did not gain too much control of any of the three interfaces, achieved the shortest spelling time for the full target sentence when using the SpellerT9. As for the other two participants, they made very few mistakes, as their spelling times were slightly longer than the minimum required, regardless of the speller they used.

The average spelling time for the full target sentence was 650.5 s, 1115.5 s and 1849.5 s when using the SpellerT9, the SpellermodPred and the Spellermod, respectively. The average spelling times for each word when using each of the three interfaces are shown in Figure 5. These results strongly suggest that SpellerT9 system was the fastest writing interface of all three.

Furthermore, our study supports the usefulness of a text predictive system irrespective of matrix size, as participants achieved shorter spelling times when using the SpellermodPred than when using to conventional interface of the Spellermod.

### 4 CONCLUSIONS

The objective of this study was to propose and to validate a new P300-based BCI speller system aimed at increasing the user’s writing speed. The proposed speller (i.e., SpellerT9) was based on the T9 interface developed for mobile phones. It presented a 4 x 3 virtual keyboard and incorporated the T9 text predictive system.

Although the study has been carried out with a very small sample, our preliminary results suggest that the SpellerT9 leads to lower spelling times than those of an adaptation of the classical Farwell and Donchin speller (i.e., Spellermod), even when the latter interface is improved by adding a text predictor (i.e., SpellermodPred). The three participants in our experiment achieved the lowest spelling times when they wrote a target sequence through the SpellerT9

Table 1: Spelling times needed by the three participants to write each word of the target sentence as a function of the speller they used.

Speller	Time (s) for each word							Total time (s)
	"Experiencia"	"BCI"	"en"	"la"	"Universidad"	"de"	"Málaga"	
Participant 1								
Spellermod	414	138	103.5	103.5	621	103.5	276	1759.5
SpellermodPred	172.5	138	103.5	69	207	103.5	207	1000.5
SpellerT9	78	78	58.5	39	97.5	39	117	507
Participant 2								
Spellermod	483	345	310.5	172.5	483	103.5	276	2173.5
SpellermodPred	138	103.5	103.5	517.5	172.5	69	345	1449
SpellerT9	78	156	58.5	78	214.5	78	177	840
Participant 3								
Spellermod	414	138	103.5	103.5	414	172.5	270	1615.5
SpellermodPred	138	138	103.5	69	172.5	69	207	897
SpellerT9	78	117	78	39	97.5	39	156	604.5
A perfect user								
Spellermod	414	138	103.5	103.5	414	103.5	270	1546.5
SpellermodPred	138	103.5	103.5	69	172.5	69	207	862.5
SpellerT9	78	78	58.5	39	97.5	39	117	507

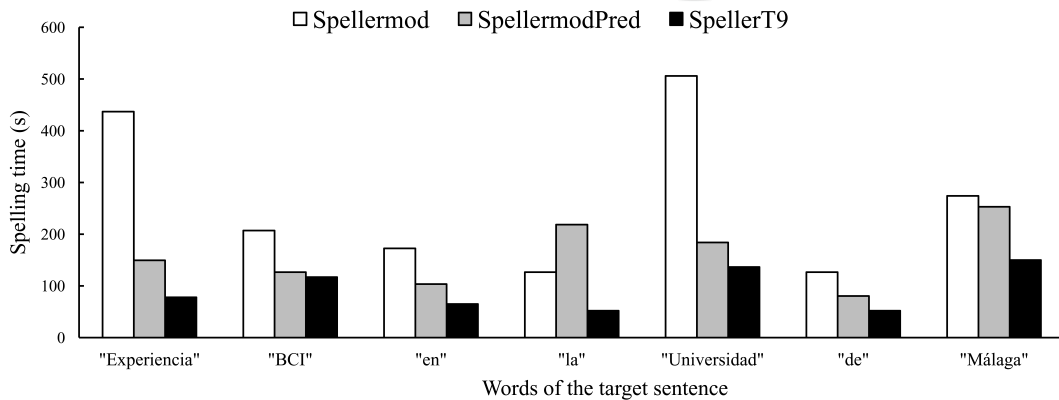


Figure 5: Average spelling times needed to write each word of the target sentence using each of the three spellers.

and the highest when they used the Spellermod. Besides, the writing times of each subject indicate that the SpellerT9 is not more difficult to use than any of the other two spellers, as participants performed just slightly worse than a perfect user.

Nevertheless, these conclusions should be supported by extending this experiment to a greater sample of participants, so that statistical tests of significance could be performed, and also by obtaining additional direct measures of user performance. Moreover, sentences of different complexity could be used

to compare the usability of these interfaces.

## ACKNOWLEDGEMENTS

This work was partially supported by the Innovation, Science and Enterprise Council of the Junta de Andalucía (Spain), project P07-TIC-03310, the Spanish Ministry of Science and Innovation, project TEC 2011-26395 and by the European fund ERDF.

## REFERENCES

- Bianchi, L., Sami, S., Hillebrand, A., Fawcett, I., Quitadamo, L., and Seri, S. (2010). Which physiological components are more suitable for visual ERP based brain-computer interface? A preliminary MEG/EEG study. *Brain Topography*, 23(2):180–185.
- Birbaumer, N. (2006). Breaking the silence: Brain-computer interfaces (BCI) for communication and motor control. *Psychophysiology*, 43(6):517–532.
- Donchin, E., Spencer, K., and Wijesinghe, R. (2000). The mental prosthesis: Assessing the speed of a P300-based brain-computer interface. *IEEE Transactions on Rehabilitation Engineering*, 8(2):174–179.
- Dunlop, M. D. and Crossan, A. (2000). Predictive text entry methods for mobile phones. *Personal Technologies*, 4(2-3):134–143.
- Farwell, L. and Donchin, E. (1988). Talking off the top of your head: toward a mental prosthesis utilizing event-related brain potentials. *Electroencephalography and Clinical Neurophysiology*, 70(6):510 – 523.
- Grover, D. L., King, M. T., and Kushler, C. A. (1998). Reduced keyboard disambiguating computer. *U.S. Patent No. 5,818,437*. Washington, DC: U.S. Patent and Trademark Office.
- Kececi, H., Degirmenci, Y., and Atakay, S. (2006). Habituation and dishabituation of P300. *Cognitive and Behavioral Neurology*, 19(3):130–134.
- Kleih, S., Nijboer, F., Halder, S., and Kübler, A. (2010). Motivation modulates the P300 amplitude during brain-computer interface use. *Clinical Neurophysiology*, 121(7):1023 – 1031.
- Kleih, S. C., Kaufmann, T., Hammer, E., Pisotta, I., Pichiorri, F., Riccio, A., Mattia, D., and Kübler, A. (in press). Motivation and SMR-BCI: Fear of failure affects BCI performance. In *Proceedings of the Fifth International BCI Meeting*.
- Krusienski, D., Sellers, E., McFarland, D., Vaughan, T., and Wolpaw, J. (2008). Toward enhanced P300 speller performance. *Journal of Neuroscience Methods*, 167(1):15 – 21.
- Lu, J., Speier, W., Hu, X., and Pouratian, N. (2013). The effects of stimulus timing features on P300 speller performance. *Clinical Neurophysiology*, 124(2):306 – 314.
- Mak, J. and Wolpaw, J. (2009). Clinical applications of brain-computer interfaces: Current state and future prospects. *IEEE Reviews in Biomedical Engineering*, 2:187–199.
- Mangun, G. R. and Buck, L. A. (1998). Sustained visual-spatial attention produces costs and benefits in response time and evoked neural activity. *Neuropsychologia*, 36(3):189 – 200.
- McFarland, D. J., Sarnacki, W. A., Townsend, G., Vaughan, T., and Wolpaw, J. R. (2011). The P300-based brain-computer interface (BCI): Effects of stimulus rate. *Clinical Neurophysiology*, 122(4):731 – 737.
- Murata, A. and Uetake, A. (2001). Evaluation of mental fatigue in human-computer interaction - Analysis using feature parameters extracted from event-related potential. In *10th IEEE International Workshop on Robot and Human Interactive Communication*, pages 630–635.
- Polich, J. and Kok, A. (1995). Cognitive and biological determinants of P300: An integrative review. *Biological Psychology*, 41(2):103 – 146.
- Schalk, G., McFarland, D., Hinterberger, T., Birbaumer, N., and Wolpaw, J. (2004). Bci2000: A general-purpose brain-computer interface (BCI) system. *IEEE Transactions on Biomedical Engineering*, 51(6):1034–1043.
- Sellers, E. W. and Donchin, E. (2006). A P300-based brain-computer interface: Initial tests by ALS patients. *Clinical Neurophysiology*, 117(3):538 – 548.
- Sellers, E. W., Krusienski, D. J., McFarland, D. J., Vaughan, T. M., and Wolpaw, J. R. (2006). A P300 event-related potential brain-computer interface (BCI): The effects of matrix size and inter stimulus interval on performance. *Biological Psychology*, 73(3):242 – 252.
- Shih, J. J., Townsend, G., Krusienski, D. J., Shih, K. D., Shih, R. M., Heggeli, K., Paris, T., and Meschia, J. F. (2013). Comparison of checkerboard P300 speller vs. row-column speller in normal elderly and aphasic stroke population. Paper presented at the Fifth International Brain-Computer Interface Meeting, Asilomar Conference Grounds, Pacific Grove, CA. Retrieved from <http://castor.tugraz.at/doku/BCIMeeting2013/020.pdf>.
- Wang, C., Guan, C., and Zhang, H. (2005). P300 brain-computer interface design for communication and control applications. In *27th Annual International Conference of the Engineering in Medicine and Biology Society IEEE-EMBS 2005*, pages 5400–5403.
- Wolpaw, J. R., Birbaumer, N., McFarland, D. J., Pfurtscheller, G., and Vaughan, T. M. (2002). Brain-computer interfaces for communication and control. *Clinical Neurophysiology*, 113(6):767–791.